

Human CDCP1 ELISA Kit

(Catalog Number: 31C010)

For the quantitative determination of human CDCP1 concentrations in serum, plasma or cell culture supernate samples

IMD (Hong Kong)

Address: Unit 513, 5/F, Biotech Centre 2, No. 11 Science Park West Avenue,
Hong Kong Science Park, Sha Tin, Hong Kong

Website: www.immunodiagnostics.com.hk

Email: info@immunodiagnostics.com.hk

Tel: (+852) 3502 2780

IMD (Canada)

Address: 3330 Bayview Avenue, Block #6, Toronto, M2M 3R8, Ontario, Canada

Email: info@immunodiagnostics.ca

Tel: +1-437-886-5136

TABLE OF CONTENTS

Contents	Page
INTRODUCTION	1
PRINCIPLE OF THE ASSAY	1
INTENDED USE	1
REAGENTS SUPPLIED	1
OTHER MATERIALS REQUIRED, BUT NOT PROVIDED	1
STORAGE	2
PREPARATION OF REAGENTS	2
PREPARATION OF STANDARDS AND SAMPLES	2
ASSAY PROCEDURE	3
CALCULATION	3
TYPICAL STANDARD CURVE	4
ASSAY CHARACTERISTICS	4
REFERENCES	5
SUMMARY OF ASSAY PROCEDURE	5

INTRODUCTION

CDCP1, also known as SIMA135, is a novel 140 kDa type I transmembrane glycoprotein with three CUB protein-protein interaction domains in its 635 aa extracellular region. The cytoplasmic region with 148 aa contains canonical phosphorylation sites for Src kinase family members and binding sites for SH3 domains. A secreted 310 aa residue variant of CDCP1 is also present by alternative splicing. It is also possible for the type I membrane CDCP1 to undergo proteolytic cleavage at its amino-terminal region, which is around 265 aa long. CDCP1 is present on the surface of epithelial and bone marrow-derived stem cells.^{1,2} The extracellular regions of mouse CDCP1 and human CDCP1's are 84% identical in terms of amino acids.

PRINCIPLE OF THE ASSAY

This assay is a quantitative sandwich enzyme-linked immunosorbent assay (ELISA). The microtiter plate is pre-coated with a polyclonal antibody specific for human CDCP1. Standards and samples are pipetted into the wells and any human CDCP1 present is bound by the immobilized antibody. After washing away any unbound substances, a biotin labelled polyclonal antibody specific for human CDCP1 is added to the wells. After wash step to remove any unbound reagents, streptavidin-horseradish peroxidase conjugate (STP-HRP) is added. After the last wash step, an HRP substrate solution is added and color develops in proportion to the amount of human CDCP1 bound initially. The assay is stopped, and the optical density of the wells is determined using a microplate reader. Since the increases in absorbance are directly proportional to the amount of captured human CDCP1, the unknown sample concentration can be interpolated from a reference curve included in each assay.

INTENDED USE

This Human CDCP1 ELISA kit is designed for quantification of human CDCP1 in serum, plasma and cell culture supernate samples.

REAGENTS SUPPLIED

Each kit is sufficient for one 96-well plate and contains the following components:

1. Microtiter Strips (96 wells), coated with a polyclonal antibody against human CDCP1, sealed
2. 10×Wash buffer, 50 mL
3. 5×Assay buffer, 20 mL
4. 100×Detection antibody solution, a biotin labelled polyclonal antibody against human CDCP1, 0.12 mL
5. Mouse CDCP1 standard, 2 ng of recombinant human CDCP1, lyophilized
6. 200×STP-HRP solution, 0.06 mL
7. Substrate solution, 12 mL, ready for use
8. Stop solution, 12 mL, ready for use
9. Sample diluent, 13mL, ready for use

Website: www.immunodiagnostics.com.hk

E-mail: info@immunodiagnostics.com.hk(HK) /info@immunodiagnostics.ca(Canada)

Tel: +852 3502 2780 (HK) / +1-437-886-5136 (Canada)

OTHER MATERIALS REQUIRED, BUT NOT PROVIDED

1. Pipettes and pipette tips
2. 96-well plate or manual strip washer
3. Buffer and reagent reservoirs
4. Paper towels or absorbent paper
5. Plate reader capable of reading absorbency at 450 nm
6. Distilled water or deionized water

STORAGE

The kit should be stored at 2-8°C upon receipt, and all reagents should be equilibrated to room temperature before use. Remove any unused antibody-coated strips from the human CDCP1 microtiter plate, return them to the foil pouch and re-seal. Once opened, the strips may be stored at 2-8°C for up to one month.

PREPARATION OF REAGENTS

Bring all reagents and materials to room temperature before assay.

A. 1×Assay buffer

Prepare 1×Assay buffer by mixing the 5×Assay buffer (20 mL) with 80 mL of distilled water or deionized water. If precipitates are observed in the 5×Assay buffer bottle, warm the bottle in a 37°C water bath until the precipitates disappear. The 1×Assay buffer may be stored at 2-8°C for up to one month.

B. 1×Wash buffer

Prepare 1×Wash buffer by mixing the 10×Wash buffer (50 mL) with 450 mL of distilled water or deionized water. If precipitates are observed in the 10×Wash buffer bottle, warm the bottle in a 37°C water bath until the precipitates disappear. The 1×Wash buffer may be stored at 2-8°C for up to one month.

C. 1×Detection antibody solution

Spin down the 100×Detection antibody solution briefly and dilute the desired amount of the antibody 1:100 with 1×Assay buffer, 100 µL of the 1×Detection antibody solution is required per well. Prepare only as much 1×Detection antibody solution as needed. Return the 100×Detection antibody solution to 2-8°C immediately after the necessary volume is removed.

D. 1×STP-HRP solution


Spin down the 200×STP-HRP solution briefly and dilute the desired amount of the 200×STP-HRP solution 1:200 with 1×Assay buffer, 100 µL of the 1×STP-HRP solution is required per well. Prepare only as much 1×STP-HRP solution as needed. Return the 200×STP-HRP solution to 2-8°C immediately after the necessary volume is removed.

PREPARATION OF STANDARDS AND SAMPLES

Human CDCP1 Standards: Reconstitute the lyophilized standard with 1 mL of Sample diluent to generate a standard stock solution of 2 ng/mL. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Pipette 500 µL of Sample diluent to 1, 0.5, 0.25, 0.125, 0.062, 0.031 ng/mL tubes. Use the standard stock solution to produce a serial dilution as shown below.

Website: www.immunodiagnosics.com.hk

E-mail: info@immunodiagnosics.com.hk(HK) /info@immunodiagnosics.ca(Canada) 2
Tel: +852 3502 2780 (HK) / +1-437-886-5136 (Canada)

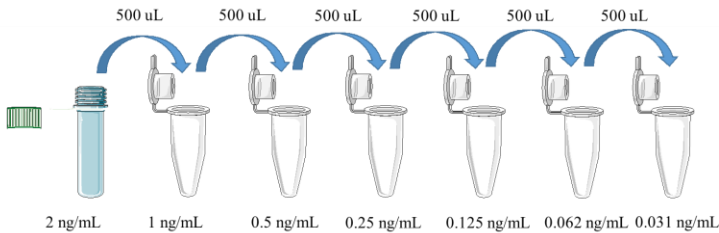

Sample diluent serves as the zero standard (0 pg/mL). The reconstituted standard stock should be aliquoted and stored at -80°C for up to one month. Avoid repeating freezing/thawing cycles. Please do not store the diluted standard solutions.

Sample Preparation:

Serum or plasma sample generally requires a **4-fold** dilution in the Sample diluent. It is recommended that the users establish their own dilution factors based on the concentration range of their samples.

ASSAY PROCEDURE

It is recommended that all standards and samples be assayed in duplicate.

1. Add 100 μL of standard or sample per well, incubate at room temperature for 1 hours.
2. Discard the content and tap the plate on a clean paper towel to remove residual solution in each well. Add 300 μL of 1 \times Wash buffer to each well and incubate for 1 minute. Discard the 1 \times Wash buffer and tap the plate on a clean paper towel to remove residual wash buffer. Repeat the wash step for a total 3 washes.
3. Add 100 μL of 1 \times Detection antibody solution to each well, incubate at room temperature for 1 hour.
4. Wash each well 3 times as in step 2.
5. Add 100 μL of 1 \times STP-HRP solution to each well, incubate at room temperature for 20 minutes.
6. Wash each well 4 times as described in step 2.
7. Add 100 μL of Substrate solution to each well, incubate at room temperature for 15 minutes. **Protect from light.**
8. Add 100 μL of Stop solution to each well, gently tap the plate frame for a few seconds to ensure thorough mixing.
9. Measure absorbance of each well at 450 nm immediately.

CALCULATION

1. Subtract the absorbance of the blank from that of standards and samples.
2. Generate a standard curve by plotting the absorbance obtained (y-axis) against human CDCP1 concentrations (x-axis). The best fit line can be generated with any curve-fitting software by regression analysis. Any curve of 4-parameter or log-log curve fitting can be used for calculation.

Website: www.immunodiagnostics.com.hk

E-mail: info@immunodiagnostics.com.hk(HK) /info@immunodiagnostics.ca(Canada) 3
 Tel: +852 3502 2780 (HK) / +1-437-886-5136 (Canada)


- Determine human CDCP1 concentration of samples from standard curve and multiply the value by the dilution factor.

TYPICAL STANDARD CURVE

The following standard curve is provided for demonstration only. A standard curve should be generated for each set of sample assay.

Human CDCP1 (ng/mL)	Absorbance (450 nm)	Blanked Absorbance
0	0.125	0
0.031	0.217	0.092
0.062	0.248	0.123
0.125	0.415	0.290
0.25	0.603	0.478
0.5	1.012	0.887
1	1.745	1.620
2	2.895	2.770

Human CDCP1 standard curve (4-parameter)

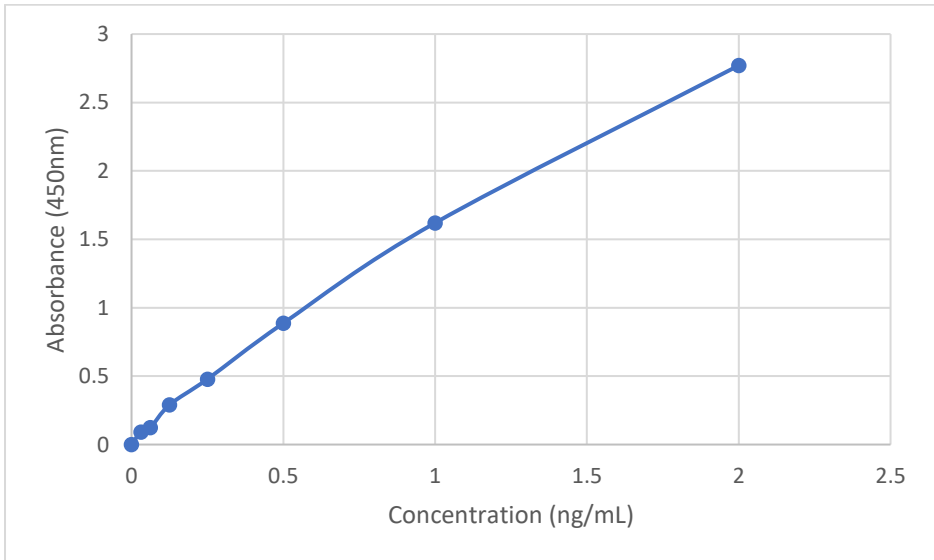

ASSAY CHARACTERISTICS

A. Sensitivity

Website: www.immunodiagnostics.com.hk

E-mail: info@immunodiagnostics.com.hk(HK) / info@immunodiagnostics.ca(Canada) 4

Tel: +852 3502 2780 (HK) / +1-437-886-5136 (Canada)

The lowest level of human CDCP1 that can be detected by this assay is 0.031 ng/mL.

B. Precision

Intra-assay Precision (Precision within an assay) C.V. <2.9%.

Inter-assay Precision (Precision between assays) C.V. <6.1%.

REFERENCES

1. He Y., et al. (2016) *Oncogene*, 35(4):468-78
2. Donders R., et al. (2017) *Stem Cells Dev.*, 15;27(2):65-84

SUMMARY OF ASSAY PROCEDURE

